

CERA-STAT™

Smart Diagnostics for Point-of-Care!

HbA1c
CRP
Glucose
Hemoglobin
Lactate



CERA-STAT™ 4000

- The one special multi-parameter Point-of-Care (POC) instrument that covers the constantly expanding range of applications with the highest precision.
- Created for the measurement of HbA1c, CRP, Glucose, Hemoglobin, Lactate, and more to come. (Glycated Albumin, u-Albumin, Creatinine, Uric Acid, Cholesterols)

The high accuracy POC analyzer that delivers lab. quality results!

Fast

Results in less than 3 minutes only

Reliable

Lab. quality accuracy and precision
Certification - NGSP, IFCC, ISO

Cost-Effective

Minimum running cost




Touch screen

High resolution, full color LCD touch screen. Easy access to operation.



Loading

Eliminate erroneous results by simple cartridge insert on auto-loading tray.

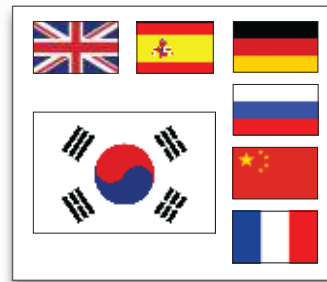

Voice Guide

Easy access with simple GUI and clear multilingual voice guide.



Specifications

Display and User Interface	Touch Screen (3.5 inch)
Detection Methodology	Optical Reflectance
Temperature Range	10 ~ 40°C / 50 ~ 104°F
Memory	300 Tests
Operation Condition	Temp.: 20~25°C / Humi.: 15~75%
Dimension	178 X 195 X 77(mm)
Weight	730g (instrument only)



► IT Connectivity



- USB / RS-232C
- LIS Compatible
- Software Update

► Built-in Thermal Printer



No need to purchase printer separately.

◀ Patient ID / Operator ID

Retrieve Patient ID (PID) and Operation ID (OID) with key-in and bar-code scanner.



◀ Quality Management

Easy quality control with control solution.



► Pipette Guide



Easy and safe handling of samples by simple pipetting guide.

► Parameter Extension Module



Extend 3 more parameters (Glucose, Hemoglobin, Lactate).

CERA-STAT™ HbA1c Test Kit

Features & Benefits



• Gold Standard!

- Boronate Affinity Principle
- HPLC (Tosoh G8) Calibrated
- NGSP (DCCT-traceable) and IFCC certified



• Fast & Cost-Effective!

- Total assay time less than 3 minutes
- High throughput - more than 50 tests/hour
- Minimal running cost



• Accurate & Reliable!

- Precision CV(%) < 3% (Guideline: < 5%)
- More than 50 countries' market proven performance



• Wide Measurement Range!

- 3 ~ 15 % (9~140mmol/mol)
- Hematocrit compensation




Test Kit Specifications


Principle	Boronate Affinity Chromatography
Total Assay Time	Less than 3 minutes
Test Range	3 ~ 15% (9~140 mmol/mol)
Sample Type	Whole Blood (Capillary or Venous)
Sample Volume	5 μ l
Storage Condition	2 ~ 8 $^{\circ}$ C

Test Principle

- The CERA-STAT™ HbA1c Test Kit utilizes a boronate affinity assay.

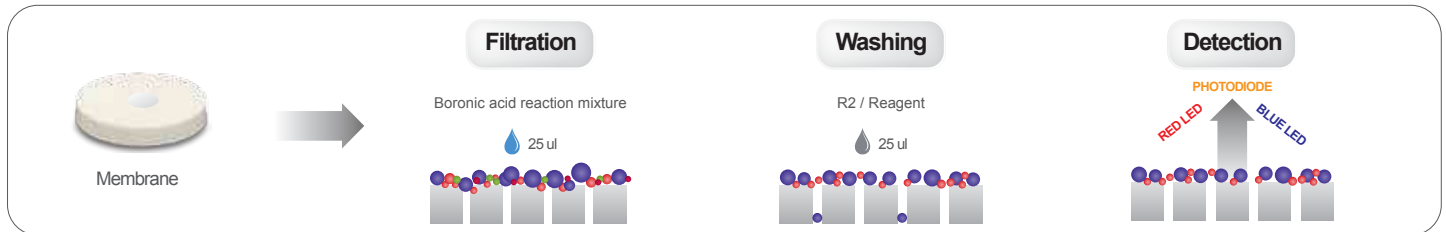

Test Procedure

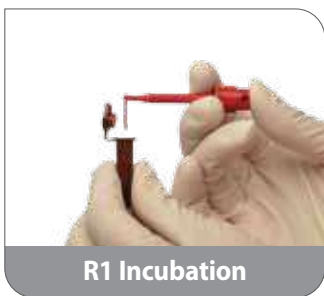

R1 Incubation

Mix well 5uL whole blood with R1 reagent and incubate for 2 minutes.



R1 mixture dropping

Apply 25uL of R1 mixture to the test device.



R2 Dropping

Apply 25uL washing solution to the Test Device (TD).




Insert the test device

Read the result within 7 seconds.


The Importance of HbA1c

HbA1c test is an important blood test used to determine how well the diabetes is being controlled. (Development and progression of diabetes complications, admissions to hospital, quality of life, mortality.)

if **1% of HbA1c** is lowered,

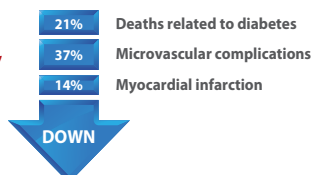

Diagnosis of Diabetes Using HbA1c

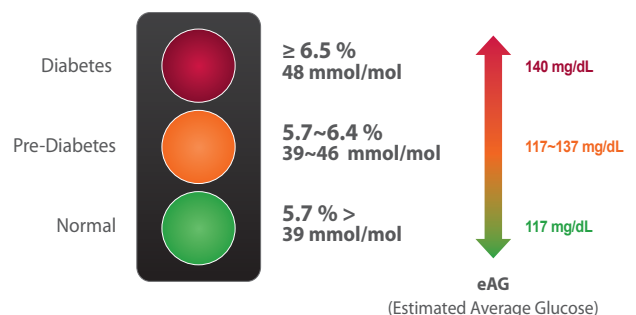

CERA-STAT™ CRP Test Kit

Features & Benefits



• Lab. Instrument Calibrated!

- Olympus AU 400
- Standardized against the IFCC/BRC/CAP protein reference material ERM-DA470 (CRM 470)



• Sample Type Free!

- No need to select sample type
- Whole blood / Plasma / Serum



• Fast & Easy!

- Total assay time less than 1 minute
- Immediate test result feedback



• Cost-Effective!

- Implemented with HbA1c in 1 analyzer
- Minimum running cost




Test Kit Specifications

Principle	Immunoassay (Optical Reflectance)
Total Assay Time	Less than 1 minute
Test Range	3 ~ 220 mg/L
Sample Type	Whole blood, Serum, Plasma
Sample Volume	5 μ l
Storage Condition	2 ~ 8 °C

Test Principle

-The CERA-STAT™ CRP Test Kit is based on an immunoassay (membrane flow-through method).

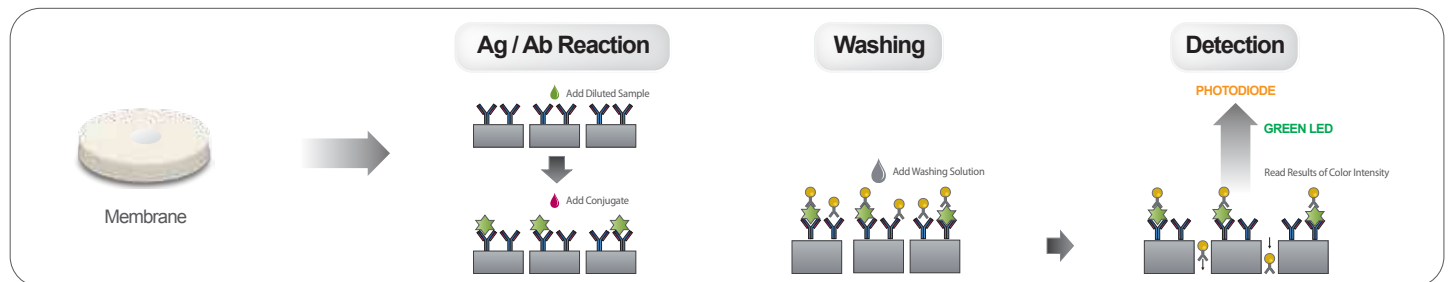

Test Procedure



Sample Dilution

Mix well 5uL blood with R1 reagent.



R1 mixture dropping

Apply 25uL of R1 mixture to the test device.



R2 Dropping

Apply 25uL of R2 reagent the test device.



R3 Dropping

Apply 1 drop of R3 reagent the test device.



Insert the test device


Read the result in 10 seconds.

The Importance of CRP

As elevated CRP levels are always associated with pathological change, the CRP assay provides information for the diagnosis, therapy and monitoring of inflammatory disease.

Importantly from a diagnostic point of view, high readings are usually seen in bacterial infection, but only low to moderate levels in viral. CRP levels reflect inflammatory activity during treatment, remission and recurrence of the disease. With follow-up CRP Testing, the course of the illness and the efficacy of any antibiotic can therefore be monitored.

Diagnosis Using CRP

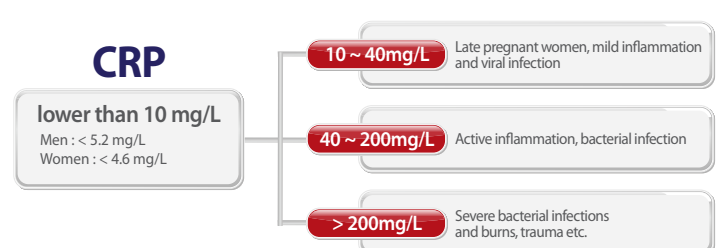

CERA-STAT™ HbA1c Test Kit

• Within-Run Precision Testing (Venous Blood)

- Each of the samples was measured 30 times per each for precision

Value	Mean HbA1c (%)	CV (%)
Normal	5.5	2.1
Intermediate	8.6	2.2
Elevated	11.3	1.8

• Day-to-day Precision Testing (Control Solution)



- Each sample was measured 10 times a day for 20 days using 3 meters across multiple lots.

Value	Mean HbA1c (%)	CV (%)
Normal	5.5	2.4
Intermediate	8.5	2.1
Elevated	11.5	2.2

• Accuracy

- The CERA-STAT™ 4000 system was evaluated at three clinical sites from 120 patients.

- The results show high accuracy and excellent correlation.

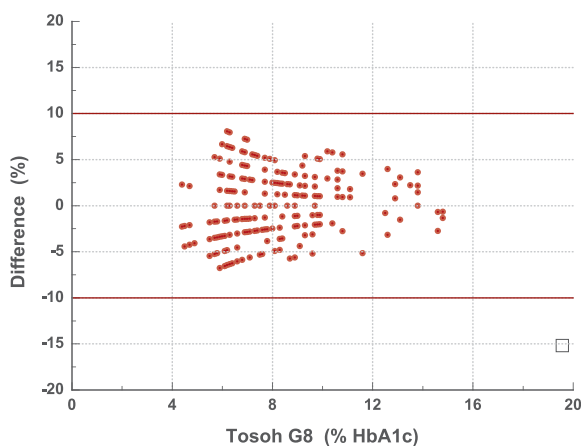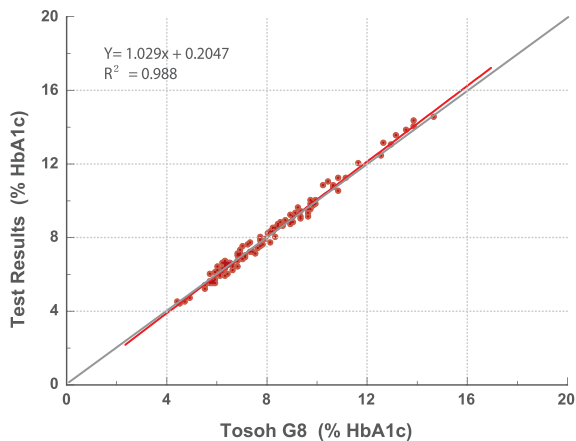

CERA-STAT™ CRP Test Kit

• Within-Run Precision Testing (Venous Blood)

- Each of the samples was measured 30 times per each for precision

Value	Mean CRP (%)	CV (%)
Normal	9.5	5.4
Intermediate	50.1	4.9
Elevated	99.7	3.6

• Day-to-day Precision Testing (Control Solution)



- Each sample was measured 10 times a day for 20 days using 3 meters across multiple lots.

Value	Mean CRP (%)	CV (%)
Normal	9.7	5.9
Intermediate	50.3	4.8
Elevated	98.8	5.1

• Accuracy

- The CERA-STAT™ 4000 system was evaluated at three clinical sites from 86 patients.

- The results show high accuracy and excellent correlation.

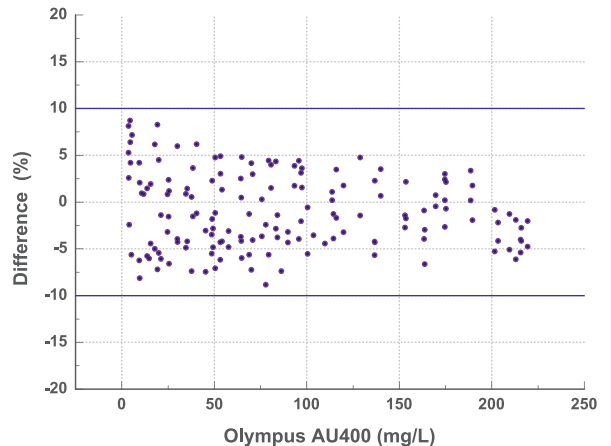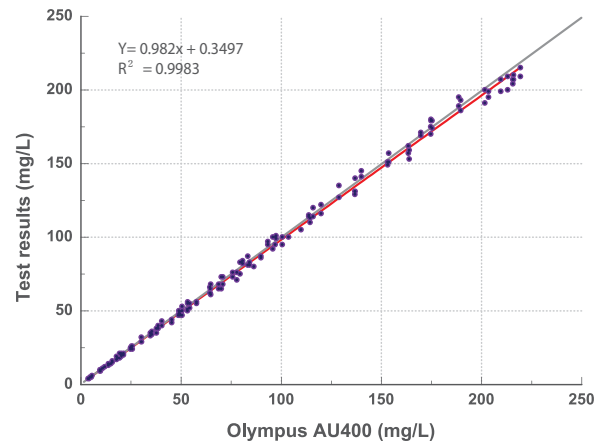

Add More Parameters




- The one special multi-parameter Point-of-Care (POC) instrument that covers the constantly expanding range of applications with the highest precision.
- Created for the measurement of HbA1c, CRP, Glucose, Hemoglobin, Lactate, and more to come. (Glycated Albumin, u-Albumin, Creatinine, Uric Acid, Cholesterols)



GHL Module



Specifications

<input type="checkbox"/> Higienic <input checked="" type="checkbox"/> Convenient <input checked="" type="checkbox"/> Customizable <input checked="" type="checkbox"/> Preferred			
Parameters	Glucose	Hemoglobin	Lactate
Enzyme	GDH - FAD	N/A	Lactate Oxidase
Test Range	10 ~ 900 mg/dL	5 ~ 26 g/dL	0.5 ~ 25 mmol/L
Unit	mg/dL (mmol/L)	g/dL	mmol/L (mg/dL)
Test Time	5 Sec	5 Sec	10 Sec
Sample Volume	0.5 ul	1 ul	1 ul
Sample Type	Capillary, Venous, AST	Capillary, Venous,	Capillary, Venous,
Hematocrit Range	10 ~ 70 %	20 ~ 60 %	20 ~ 60 %
Calibration	Autocode	Code-Key	Code-Key
Expiry Date (After Opening)	4 months	3 months	3 months
Shelf Life	24 months	18 months	18 months
Storage Condition	1 ~ 32 °C	1 ~ 32 °C	1 ~ 32 °C



Test Procedure



Insert test strip.



Apply blood sample (Sip-in).



Accurate result within 5 seconds.



Order Information

Telephone +82-70-8894-2725
 Fax +82-31-455-0126
 Email marketing@ceragemmedisys.com
 Address Marketing Department
 16, Jeongja 1-gil, Seonggeo-eup, Seobuk-gu,
 Cheonan-si, Chungcheongnam-do, South Korea

► CERA-STAT™ 4000 Analyzer

Product Name	Contents
CERA-STAT™4000 Analyzer	1 analyzer 1 power adaptor 1 printer paper roll 1 user manual

► CERA-STAT™ 4000 Control solution

Product Name	Contents
CERA-STAT™ HbA1c Control Solution	2 levels x 0.5 ml/box
CERA-STAT™ CRP Control Solution	2 levels x 0.5 ml/box

► CERA-STAT™ HbA1c Test Kit

Product Name	Contents
CERA-STAT™ HbA1c Test Kit	32 tubes R1 reagent 30 units Test Device 1 vial R2 reagent

► CERA-STAT™ 4000 Accessories and Spare parts

Product Name	Contents
Pipette	1 ea (25 uL)
Capillary Tube	1 vial (200 pcs, 5uL)
Capillary Tube Holder	1 ea
Pipette Tip	1 box (96 tips)
Printer Paper	1 roll
Lancet	1 box (200 pcs)
Lancing Device	1 ea
Pipetting Guide	3 ea

► CERA-STAT™ CRP Test Kit

Product Name	Contents
CERA-STAT™ CRP Test Kit	32 tubes R1 reagent 30 units Test Device 1 vial R2 reagent 1 vial R3 reagent

